

(19) World Intellectual Property
Organization
International Bureau



(43) International Publication Date
25 March 2004 (25.03.2004)

PCT

(10) International Publication Number
WO 2004/025963 A1

(51) International Patent Classification⁷: **H04N 7/18**,
9/47, A62B 01/04

(21) International Application Number:
PCT/US2003/029012

(22) International Filing Date:
15 September 2003 (15.09.2003)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
60/410,456 13 September 2002 (13.09.2002) US

(71) Applicant: **KARL STORZ IMAGING, INC.** [US/US];
175B Cremona Drive, Goleta, CA 93117 (US).

(72) Inventor: **KENNEDY, Bruce, L.**; 311 Calle Cedro, Santa
Barbara, CA 93101 (US).

(74) Agents: **WHITMYER, Wesley, W. Jr.** et al.; St. Onge
Steward Johnston & Reens LLC, 986 Bedford Street, Stam-
ford, CT 06905-5619 (US).

(81) Designated States (*national*): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NO, NZ, OM, PH, PL, PT, RO, RU, SD, SE, SG, SK, SL, TJ, TM, TN, TR, TT, TZ, UA, UG, UZ, VN, YU, ZA, ZM, ZW.


(84) Designated States (*regional*): ARIPO patent (GH, GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HU, IE, IT, LU, MC, NL, PT, RO, SE, SI, SK, TR), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

Published:

- with international search report
- before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments

[Continued on next page]

(54) Title: VIDEO RECORDING AND IMAGE CAPTURE DEVICE

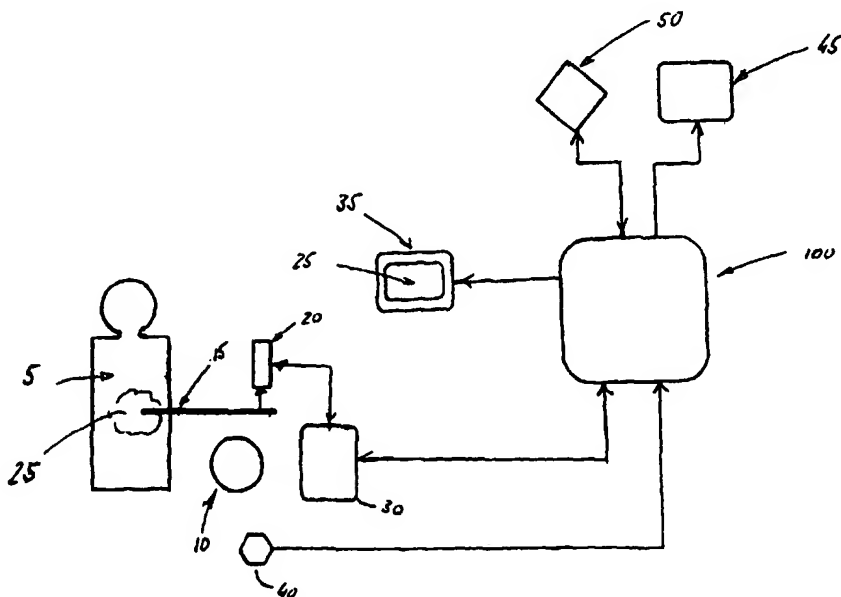

(57) Abstract: A video recording and image capture device for documenting surgical procedures that includes a main board for executing a plurality of software, a multimedia interface (100) operable to receive a video signal and process it into an MPEG layer stream, the video interface (35) connected on a first bus to the main board, a hard drive (50) to record an MPEG layer stream as a file, an optical media drive to write an MPEG layer stream as a file, the hard drive and the optical media drive operably connected on a second bus, the bus being vertically stacked and connected to the main board, and a touch screen interactive for user control, connected to the main board on a second bus to control the video interface.



For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

Title Of Invention

VIDEO RECORDING AND IMAGE CAPTURE DEVICE

Prior Application

[0001] Applicant claims priority benefits under 35 U.S.C. §119(e) of U.S. Provisional Patent Application Serial No. 60/410,456 filed September 13, 2002.

Field Of The Invention

[0002] The invention relates generally to device for video recording and image capture, and more particularly to such a device for image based documentation of surgical procedures. The invention also relates to means to process signals into an MPEG layer stream.

Background Of The Invention

[0003] The maxim that "a picture is worth a thousand words" is more true than ever in image based documentation of surgical procedures. There patients' lives and physicians' reputations are at stake. The early history of image based documentation is littered with crude attempts at utilizing photographic film to capture anatomical curiosities and

- 2 -

groundbreaking surgical advances for teaching purposes. However, little attempt was made to provide documentation of routine cases. Average patients simply did not merit this special consideration.

[0004] With the advent of analog cameras coupled to fiber optics, physicians began displaying some surgical patient images on video monitors in the operating room. This was especially true in endoscopic surgeries where physicians peer inside patients' body cavities normally only viewable with open surgery. Attempts made to systematically record all patient procedures on videotape required large and cumbersome archives of videotapes.

[0005] Although analog cameras are still used, solid state image cameras coupled to endoscopes and other medical instruments are now standard. These cameras produce images in digital format. Such format allows convenient and efficient image transfer, review, and archival.

[0006] One method for archiving digital images is suggested in U.S. Patent 6,067,075 to Pelanek. Therein, a workstation is disclosed for transferring and archiving patient images previously stored in the memory of diagnostic equipment. However, this method does not disclose

- 3 -

contemporaneously saving images in a permanent location, meaning that the equipment is subject to "downtime" as data is extracted from its memory.

[0007] Once image data has been extracted and archived it must be made available to those in a position to best make use of it, the treating physician. Ironically in a circular manner, the person to whom eventual delivery of images is made is the same person who used the diagnostic equipment to record the images in the first place who must now await it being made available to him. Thus, it would be advantageous to the physician to have the data available at the conclusion of the surgical procedure or series of surgeries. Consequently, equipment downtime for data extraction also is eliminated increasing efficiency of equipment and facility utilization.

[0008] Image data availability, however, is only of value when the data can be read and images displayed readily. Thus, exotic and unusual methods of storing and reading image data chain physicians. Most convenient are displays in NTSC and PAL standards and devices that can play image data on these displays. NTSC is the common television standard in the U.S., while PAL standards predominate in Europe and in parts of Asia. Additionally, most convenient for medical personal, is for images and video to be viewable utilizing common off-the-shelf optical media players (i.e. set-top DVD players) and/or standard personal computers.

- 4 -

[0009] U.S. Patent 5,045,955 to Ikeda discloses an apparatus coupled to a digital tape drive for recording and reproducing high-definition medical images having specific analog matrix exceeding that of NTSC or PAL standards. Typically, these images can only be produced by specialized imaging equipment and can only be viewed on highly specialized monitors. They are incompatible with NTSC or PAL standards and thus are inapplicable to the use of documenting procedures where analog or digital cameras provide a video signal to be displayed .

[0010] Other suggestions have been made to integrate images into a medical setting. Therein, imaging is primarily related to diagnosis rather than documentation; resulting in files solely consisting of visually relevant components and omitting narration by the treating physician.

[0011] Suggestions to incorporate equipment in surgical suites fail to consider issues relevant to logistics of placing equipment. Surgical suites include a plurality of equipment. Vertically stacking equipment in shelves, i.e. racking, advantageously conserves space. However, this limits the readily available user-operator access to front face plates. Equipment that incorporates space saving advantages while providing maximum user-operator access, therefore, is highly desired.

- 5 -

[00012] Therefore, what is desired is a device that produces and saves a surgical documentary recording file that incorporates both video and audio to a transportable and common media contemporaneously during the surgery.

[00013] What is also desired is a device that formats a video signal into a plurality of video formats for display, displays an image stream, and allows a user to capture still images and save same as a still graphic file to the same media as the documentary recording file.

[00014] It is further desired that the device and the parts that the user interacts with are convenient and accessible.

[00015] Also, it is desired that the device is capable of "feed through" of real-time video signals to a plurality of display devices, in a plurality of video formats, when the device is in a standby mode, when the device is off, or in the event when the device malfunctions.

[00016] Further, what is desired is an interactive tutorial which allows a user to manipulate the files saved.

[00017] These and other objectives are met by the embodiments of the present invention.

- 6 -

Summary Of The Invention

[00018] In accordance with one embodiment, a device for medical video recording includes an endoscope, and an imager for converting energy such as electromagnetic energy, direct current energy and the like, which is received from said endoscope to signals that are contemporaneously stored onto said media.

[00019] In accordance with one embodiment of the invention, a device is provided that encodes a video signal into a documentary recording file formatted in an MPEG-2 layer.

[00020] In accordance with one embodiment of the invention, a multimedia interface to process a video signal and audio signal into a first and second digital data stream having common characteristics is provided.

[00021] In accordance with one embodiment of the invention, a recording mode for recording a video stream during a surgical procedure is provide for surgical documentation.

[00022] In accordance with one embodiment of the invention, a means for a video signal to be displayed by a display unit during recording

- 7 -

mode, or when the device is in a standby mode, or when the device is off, or when the device has malfunction, is provided.

[00023] In accordance with one embodiment of the invention, an archival mode is provided for review, edit and playback of a documentary recording file and graphic file.

[00024] In accordance with one embodiment of the invention, a medical instrument having touch screen control includes a touch screen for entering control commands, a processor for receiving the control commands and for generating control signals to operate the medical instrument, a housing for enclosing the processor. The touch screen is movable between a first position protected by the housing and second position extended from the housing for entry of the control commands.

[00025] In accordance with one embodiment of the invention, a multimedia interface for processing a video signal for recording video into a multiple frame layer includes a controller for an inter-ic bus for providing a multiple master digital connection, an analog to digital converter for converting a video signal to a first digital stream, the converter operably connected to the inter-ic bus, a video compression and decompression integrated circuit for encoding the first digital stream into a second digital

- 8 -

stream having frames and decoding a second digital stream, the video compression and decompression integrated circuit operably connected to the inter-ic bus a programmable buffer for selectively saving frames handled by the controller, the buffer operably connected to the controller and the video compression and decompression integrated circuit and the buffer inserting the frame into the second digital stream for decoding.

[00026] In accordance with one embodiment of the invention, a method for recording an MPEG layer file for documenting surgical procedures while displaying an MPEG layer stream and n number selecting still image files corresponding to the MPEG layer stream, includes the steps of providing a first digital data stream comprising a video signal, providing a second digital data stream comprising an audio signal, multiplexing an MPEG layer data stream from the first and second digital data stream, streaming the MPEG layer data stream to a hard drive and an optical media drive operably connected on a vertically stacked bus, writing the MPEG layer stream to the hard drive and the optical media drive, displaying the MPEG layer stream on a display unit, selecting n number of frames from the MPEG layer stream, converting n frames to n still image files, and multiplexing the output signal to the display unit by adding n still image files.

- 9 -

[00027] The terms "communicate", "communicating" and "communication" as used herein include both conveying data from a source to a destination, as well as delivering data to a communications medium, system or link to be conveyed to a destination. The term "communication" as used herein means the act of communicating or the data communicated, as appropriate.

[00028] The invention and its particular features and advantages will become more apparent from the following detailed description considered with reference to the accompanying drawings.

Brief Description Of The Drawings

[00029] Fig. 1 is a schematic diagram of a Video Recording and Image Capture Device used in a surgical patient setting in accordance with the present invention;

[00030] Fig. 2 depicts a front panel elevation view of a Video Recording and Image Capture Device of Fig. 1;

[00031] Figs. 3 depicts a rear panel elevation view of a Video Recording and Image Capture Device of Fig. 1;

- 10 -

[00032] Fig. 4 is a schematic diagram of a Video Recording and Image Capture Device of Fig. 1;

[00033] Figs. 5a, 5b, and 5c depict a Video Recording and Image Capture Device of Fig. 1;

[00034] Fig. 6 is a schematic diagram of a multimedia interface of Fig. 1;

[00035] Fig. 7 depicts a schematic of interconnecting Video Recording and Image Capture Device and a display unit of Fig. 1;

[00036] Figs. 8 through 13 depict use of a Video Recording and Image Capture Device through the interactive display of the touchscreen of Fig. 1;

[00037] Fig. 14a and 14b depict a plan view a track advance system for a touchscreen of a Video Recording and Image Capture Device of Fig. 1; and

[00038] Fig. 15 depict a Video Recording and Image Capture Device of Fig. 1 with touch screen fully retracted, touch screen extended and touch screen extended and deflected.

- 11 -

Detailed Description Of The Drawings

[00039] The present invention will be described as used in connection with one or more endoscopes. It will be understood that other applications may be used equally effectively. Various frame displays and icons having particular graphical representations are described in connection with the functions of the present invention. It will be understood that other graphical representations may be used equally effectively in communicating to users the function performed therein.

[00040] Herein, image and image stream refer to the perception of the user utilizing their audiovisual capabilities; an image stream may also include an auditory component. Video signal, digital signal, analog signal, data stream, or the like refer to electrical signals in the present invention and electrical equipment operably connected and/or associated with the present invention.

[00041] Fig. 1 is a schematic diagram of a Video Recording and Image Capture Device used in a surgical patient setting in accordance with one embodiment of the present invention. Patient 5 is being examined by user 10 with an endoscope 15. User 10 may be a physician, surgeon, nurse, or other qualified professional or para-professional. Video Recording and

- 12 -

Image Capture Device (imager) **100** has been placed into a video recording mode. A camera head **20**, such as a charge coupled device (CCD), CMOS, or CCI chip, is coupled to endoscope **15** to receive and produce a video signal **300** (see Fig. 4) of a body cavity of patient **5**. Video signal **300** results in an image stream **25** when displayed on a display unit.

[00042] As user **10** manipulates endoscope **15**, user **10** controls camera head **20** with camera control unit (CCU) **30** and observes image stream **25** on a display unit, for example external video screen **35**. Imager **100** is operably connected to CCU **30** to receive video signal **300**. Device is also operably connected to external video screen **35**, microphone **40**, printer **45**, and network **50** through standard ports. In one embodiment, imager **100** is operably connected to camera head **20** to receive video signal **300** and control camera head **20**, obviating the need for CCU **30**.

[00043] As user **10** examines and treats patient **5**, imager **100** is recording a digital data stream representing image stream **25** on optical media drive (OMD) **125** (see Fig. 2) and saving a backup copy to hard drive (HDD) **120** (see Fig. 4) for a plurality of purposes. During this period user **10** may provide narration to the examination. Microphone **40** or an independent audio recording system captures the narration and converts it into audio

- 13 -

signal **314i** (see Fig. 6) or **316i** (see Fig. 6), respectively, collectively audio signal **315** (see Fig. 6).

[00044] Upon encountering a situation requiring further investigation, user **10** utilizes an image capture mode to save and freeze a first image from image stream **25** for further investigation. Using imager **100**, a second image substantially like the first image can be superimposed on image stream **25**. Upon encountering further situations that attracts the attention of user **10**, a plurality of second images substantially corresponding to respective first images found of interest can be saved and concurrently superimposed on image stream **25**. A file corresponding to second image can be printed with printer **45** and/or forwarded over network **50** to other persons for consultation.

[00045] Figs. **2** and **3** depict a front panel and rear panel elevation view, respectively, of a Video Recording and Image Capture Device in accordance with one embodiment of the present invention. Fig. **4** is a schematic diagram of a Video Recording and Image Capture Device in accordance with one embodiment of the present invention. Imager **100** is substantially housed in chassis **105** and includes a plurality of components: power supply **110**, microprocessor main board (MMB) **115**, hard drive (HDD) **120**, optical media drive (OMD) **125**, communication interface **130**, multimedia interface **135**, speaker **140**, digital video interface **150**. Chassis

- 14 -

105 includes an add-on tray **105a** that advantageously houses touchscreen **145**.

[00046] Power supply **110** is connected to an AC power supply with an electric cord at power port **110a** located on chassis back panel **105b**. When power switch **110b** of chassis front panel **105c** is engaged, power supply **110** provides suitable power to components of imager **100**. Power supply **110** conforms to IEC 601-1 isolation requirements, provides power meeting medical grade standards of 145 Watts, includes a power correction factor, and is capable of automatically handling automatically an AC voltage range of 100 to 250 VAC, 50-60 Hz.

[00047] Microprocessor main board (MMB) **115** executes software and includes a central processor unit ("processor"), random access memory, a plurality of expansion slots, a BIOS chip, and on-board sound and graphics capabilities on a footprint convenient for chassis **105**. Therein, it may be that an Intel Pentium III with a processing speed of at least 800 MHz; an Intel 815 chip set; at least three (3) PCI and one (1) AGP slot; SDRAM of at least 128 MB; on-board AGP graphics; and a flash upgradeable BIOS chip wherein a customized logo may be loaded, is provided on an ATX motherboard. Further, MMB **115** preferably includes port panel **115a** to connect to other devices and or networks via serial, parallel, USB and ethernet, and to connect

- 15 -

to mouse, keyboard, and video monitor; a Intel 40-pin DVO motherboard connector, or similar, and support for the connector.

[00048] Hard drive (HDD) **120** and optical media drive (OMD) **125** maybe IDE or Enhanced IDE (alternatively IDE) compatible data storage media drives operably connected MMB **115** by a vertically stacked IDE bus **116**. HDD **120** maybe a magnetic hard drive having at least 40 Gigabytes of storage and minimal access time, as such a drive from Maxtor having EIDE access time of 8.0 ms, 7200 rpm disk speed is preferred. OMD **125** is preferably a DVD+RW drive capable of reading and writing data to an optical media disk, such as a compact disk (CD) and/or a digital versatile disk (DVD).

[00049] Communication interface **130** is any kind of network or proprietary communications interface. Therein, for example, a network card that is capable of interfacing with the Karl Storz®, Inc. Storz Communication Bus (SCB) is preferred.

[00050] Multimedia interface **135** connects to MMB **115** via a Peripheral Component Interconnect (PCI) local bus to provide record and write image stream **25** originating from camera head **20**. Speaker **140** is housed in chassis **105** and provides auditory capabilities for imager **100**.

- 16 -

[00051] Digital video interface **150** is operably connected to MMB **115** to create a video signal conforming to the digital visual interface (DVI) standard. Therein, a digital video interface **150** is preferably physically implemented as a printed circuit board having an Intel 40-pin DVO connector, or similar, to MMB **115** and a DVI-D output connector in expansion slot **105d**.

[00052] A touchscreen **145** is provided as illustrated on Figs. **5a**, **5b**, and **5c** in accordance with one embodiment of the present invention. A surface **145a** responsive to touch by an operator, such as user **10**, and a display **400** capable of showing the functions of imager **100** are included in touchscreen **145**. Preferred is a touchscreen manufactured by Optrex Inc. of Plymouth, MI. A video connection to MMB **115** is made to the corresponding DVI-D output and a data and power connection is made between standard RS-232 serial ports.

[00053] Touchscreen **145** is advantageously housed in tray **105a** (see Fig. 14a) of imager **100** within chassis **105**. Therein, it is mounted within a track advance system (TAS) **146** (see Fig. 14 a) so that touchscreen **145** is secure and is relatively flush with a front face of chassis **105** as depicted in accordance with one embodiment of the present invention in Fig **18**.

- 17 -

[00054] TAS 146 allows user 10 to advantageously use the space available when equipment is racked. User 10 presses a button or other releasing mechanism to release touchscreen 145 and slides touchscreen 145 away from chassis 105 and out of tray 105a as indicated by the arrows as depicted in accordance with one embodiment of the present invention in Fig. 5b. To make touchscreen 145 more user friendly and visible, user 10 is able to tilt touchscreen 145 at an angle as indicated by the arcuate arrows in accordance with one embodiment of the present invention in Fig. 5c.

[00055] Fig. 15 discloses the touch screen in various states of deployment. For example, 101 shows one embodiment in which the touch screen is fully retracted, however, other embodiments will not have the touch screen fully retract. 102 shows the touch screen extended out and 103 shows the touch screen extended out and deflected from the plane of the housing.

[00056] Figs. 14a and 14b depict a plan view of a track advance system for a touchscreen of a Video Recording and Image Capture Device in accordance with one embodiment of the present invention. A platform 144 (shown advanced out of tray 105a) disposed to tray 105a is operable with rails 143a and 143b and is guided by tracks 147a and 147b by bearings or other friction reducing mechanisms as depicted in accordance with one

- 18 -

embodiment of the present invention in Fig.14a. Releasing mechanism **143d** includes one or more components that selective to user desire, release touchscreen **145** in order to advance it. Releasing mechanism **143d** further may include one or more springs **143e**.

[00057] Platform **144** may be of any suitable design to hold touchscreen **145** even when placed at an angle from horizontal. Touchscreen **145** is operative with imager **100** through cables and connectors.

[00058] Rails **143a** and **143b** have stops **143c** (only partially shown for clarity) operable with tracks **147a** and **147b** to prevent advancing touchscreen **145** beyond a predetermined point.

[00059] TAS **146** includes on or more hinge **142**, such as edged hinge **142a** and **142b**, or center hinge **143c** a center hinge as depicted in accordance with one embodiment of the present invention in Fig.14b. Hinge **142a** and **142b** cooperate to angle platform **144** so that user **10** can during the surgery interactively access touchscreen **145**. To prevent changing angle of the platform **144** or accidental closure, one or more tapping mechanisms are disposed with hinge **142**, that make it resistant to unintentional movement.

- 19 -

[00060] Fig. 6 is a schematic diagram of multimedia interface **135** in accordance with one embodiment of the present invention. Multimedia interface **135** is physically implemented on one or more printed circuit boards, also commonly referred to as expansion cards, having a plurality of integrated circuits and a PCI bus connection **136** to MBB **115** for data transfer. Through bus **136** multimedia interface **135** also receives electric power. Audio and video connection ports, i.e. input and output ports, are physically implemented in expansion slots **105** and integrally connected to multimedia interface **135**. In one embodiment, multimedia interface **135** is implemented as a PCI expansion card with bus connection **136** to MBB **115** and a further printed circuit board connecting directly to the PCI expansion card.

[00061] Resident on multimedia interface **135** is an Inter-IC bus operatively controlled by controller **200**. Controller **200** implements the Inter-IC bus as a multi-master bus to connect circuits to PCI interface **210**. Router **220** is provided as a field programmable gate array and has programmable read only memory that is accessible via a port, such as a JTAG port.

[00062] In recording mode, imager **100** receives the input of video signal **300** and audio signal **315** and contemporaneously encodes both signals while writing the data stream to HDD **120** (see Fig. 4) and/or media in OMD **125** (see Fig. 4).

- 20 -

[00063] Video signal **300** is received by multimedia interface **135** as analog video signal **304i** or digital video signal **306i** in input ports located in expansion slot **105d** (see Fig. 3). The active input port is automatically detected by multimedia interface **135**, as are active output ports.

[00064] A relay **205** is operative to bypass video signal **300** to an exit port corresponding to the input port for display by an external monitor when imager **100** is not powered or imager **100** is in standby mode. Therein, relay **205** includes a receiver for receiving a sense signal from software to indicate that the recording mode is engaged. If the sense signal is not received with a predetermined time, video signal **300** is bypassed. If imager **100** is not powered, a default mode of relay **205** bypasses the signal to the corresponding port, i.e. video signal **300** input on the S-video input is bypassed to an S-video output port.

[00065] Analog video signal **304i** is received using composite video input or S-Video input. If analog video signal **304i** is received when imager **100** is not electrically powered or recording mode is not engaged, video signal **300** is bypassed using bypass relay **205**. Received analog video signal **304i** is digitized using analog to digital converter **240**. Therein, the NTSC or PAL standard analog video signal **304i** is digitized to first internal data stream, digital data stream (DDS) **310**. A digitized data stream having 4:2:2

- 21 -

luminance to chrominance (YUV) pixels is preferred. Other data stream configurations may also be used. In particular, a data stream having 8:2:2 YUV may be advantageously used in connection with CCU 30 (see Fig. 1) which is capable of producing higher analog video frame quality. DDS 310 is then streamed via router 220 to video media compression and decompression integrated circuit (V-codec) 230 where it is encoded.

[00066] Digital video signal 306i is received using the SDI digital video signal input. If digital video signal 306i is received when imager 100 is not electrically powered or recording mode is not engaged, video signal 300 is bypassed using bypass relay 205. Received signal 306i is processed by SDI receiver 250 and converted to a first internal data stream, DDS 310. A digitized data stream having a 4:2:2 luminance to chrominance (YUV) pixels is preferred; although other data stream configurations may also be used. DDS 310 is streamed via router 220 to V-codec 230 where it is encoded.

[00067] Inputs for audio signal 314i originating from a stereo line and audio signal 316i originating from microphone 40 are provided for recording a desired audio signal such as dictation. Both inputs may be combined to create a single audio signal 315 or used individually. Audio signal 315 is received by audio compression and decompression integrated circuit (A-codec) 260 and converted to a second internal data stream, digital data

- 22 -

stream for audio (DDSA) 312, and passed to automatic gain control 270 disposed on the Inter-IC bus. DDSA 312 is then streamed to V-codec 230.

[00068] V-codec 230 is provided as embedded software, preferably operating on a LINUX or UNIX embedded platform, on one or more integrated circuits on the Inter-IC bus and operatively connected to controller 200. Also operatively connected are one or more buffer memories, such as SDRAM integrated circuits. Configuration settings of V-codec 230 are stored on an associated erasable electronic programmable read only memory (EEPROM or EPROM) circuit, or similar. The embedded software of V-codec 230 executes an algorithm to decode and/or encode a Motion Picture Experts Group (MPEG) layer, such as MPEG, MPEG-2 and/or MPEG-4, data stream (MDS) 320. MDS 320 advantageously utilizes high compression rates achieved by using an index frame and noting a sequence of changes to that index frame in subsequent images. Therein, MDS 320 is comprised of a stream of frames 322.

[00069] Algorithms of this type are known to execute file formatting appropriate for CD-R and a plurality of DVD media storage and play. Typically, MDS 320 is preferred to encode in a file format designated as "VOB" applicable to DVD+RW media storage and play. It should be

- 23 -

appreciated that the present invention may be adapted readily to utilize other compression and decompression algorithms.

[00070] V-codec **230** multiplexes **DDS 310** and **DDSA 312** into **MDS 320** which is then streamed to **MMB 115**. From there, **MDS 320** is streamed to **HDD 120** and to **OMD 125** via vertically stacked **IDE bus 116**. Therein, **HDD 120** writes **MDS 320** to a magnetic disk and streams a copy to **OMD 125** for writing to an optical disk such as a CD-R or DVD media to create contemporaneous documentary recording file while the surgery is being conducted by user **10**. If the write process on **OMD 125** is interrupted or fails, a backup copy resides on **HDD 120** for a subsequent write attempt after the conclusion of the surgery.

[00071] A means for a video signal to be displayed by a display unit during recording mode is provided. The display unit may be external video screen **35** or touchscreen **145**. Fig. 7 depicts a schematic of interconnecting imager **100** and a display unit in accordance with one or more embodiments of the present invention. An embodiment of video screen **35**, external video screen **35a**, is operable to receive an analog and/or digital signal using connectors for S-video, composite and/or SDI format. Therein, multimedia interface **135** senses the active output port and router **220** streams **DDS 310** accordingly to either SDI transmitter **280** to produce digital video signal **306x**

- 24 -

or to digital to analog converter **290** to produce analog video signal **304x**, respectively. In converter **290**, common data stream DDS **310** is automatically converted to the appropriate NTSC or PAL standard analog signal in use by video screen **35a**.

[00072] Touchscreen **145** is operable to receive a video signal in digital visual interface (DVI) format, and an embodiment of video screen **35**, external video screen **35b** having touchscreen capabilities, is operable to receive a video signal in digital visual interface (DVI) format or analog monitor format. Therein, MMB **115** streams a copy of MDS **320** to resident AGP graphics support and/or DVI graphics support and digital video interface **150** for output to touchscreen **145** and video screen **35b** as required by the active output.

[00073] Image capture mode is provided for saving a frame **322** (see Fig. 6) from MDS **320** substantially like image of image stream **25**. User **10** views an image of interest in image stream **25** and initiates instruction to "freeze" the image of interest. Since both reaction time on behalf user **10** and processing time on behalf of imager **100** has passed when such an instruction has been received, a frame **322** substantially like image **26** is saved, wherein the substantiality is temporal. The freeze instruction is forwarded to multimedia interface **135**. Therein, controller **200** instructs PCI interface **210**

- 25 -

to forward the current frame **322** being handled to frame buffer **295**, also known as frame grabber, which stores frame **322**.

[00074] Frame buffer **295** can be implemented as an integrated circuit, capable of storing and identifying a plurality n of frames **322** corresponding to maximum number n frames capable of being stored according to the buffer size (hereinafter frame **322₁** designating the first frame **322** stored, frame **322₂** the second, . . . , and frame **322_n** the last frame stored). As shown, identification may be implemented by designating a first-in-first-out order, or similar order. Upon receipt of frame **322₁**, buffer **295** forwards a copy to router **220**. Router **220** multiplexes frame **322₁** with DDS **310** and streams the combined signal to the active output port for display as combined image. As described further herein in connection with image capture mode, user **10** is able to manipulate the position and size of the combined image within image stream **25** and on a display unit.

[00075] A copy of frame **322₁** is saved to HDD **120**, preferably in file format Joint Picture Experts Group JPEG layer corresponding to the MPEG layer such as MPEG, MPEG-2 and/or MPEG-4 layer, as a graphic file. A software application for conversion to other formats such as "TIFF," "BMP," and/or "FPX", or similar, is provided.

- 26 -

[00076] Upon additional instruction by user **10** to capture further images, further corresponding frames **322** are saved in the manner described. Therein, frame **322₂** is multiplexed with frame **322₁** and DDS **310** and the combined signal streamed to the active output for display on a display unit.

[00077] An archival mode is provided for review, edit and playback of documentary recording file and a graphic file. Therein, the recording file is accessed and a digital data stream corresponding to MDS **320** is read from media of HDD **120** and/or OMD **125** and is streamed to V-codec **230** and is decompressed into a digital data stream corresponding to DDS **310**. The decompressed digital data stream is then routed to the active port for display or transferred to MMB **115** for display on a display unit.

[00078] Figs. **8** through **13** depict use of imager **100** through interactive display **400** of touchscreen **145** in accordance with one embodiment of the present invention. It should be appreciated that similar usage is achieved through use of other input devices, as for example mouse and keyboard, coupled to a display unit.

[00079] Upon powering of imager **100**, it is in standby mode and page **410** is shown as depicted in Fig. **8** in accordance with one embodiment

- 27 -

of the present invention. Display 400 is shown as page 410 providing a plurality of fields. The fields depicted include fields grouped to display surgical information 600, multimedia status 610, image panel 620, and control panel 630. In the embodiment illustrated, multimedia status 610 indicates that the optical media includes data saved from a previous surgical session. To use imager 100 for the current session and input patient data, user 10 touches the desired field in surgical information block 600 to include the requisite data.

[00080] Surgical information block 600 includes fields for biographical patient information, identity of treating physician, and additional information as may be convenient and necessary. If the field requires an alpha-numeric entry, alpha-numeric keyboard page 420 is displayed on top of page 410, as depicted in Fig. 9. User 10 enters the data by touch. Field 422 contemporaneously displays the entry made. The user confirms the entry and is taken back to page 410 to make the next selection. If the desired field of frame 410 requires a numeric entry, numeric keyboard page 430 is displayed on top of page 410, as depicted in Fig. 10 according to one embodiment of the present invention. User 10 enters the data by touch. Field 422 contemporaneously displays the entry made. The user confirms the entry and is taken back to page 410, now modified with additional data as

- 28 -

depicted in Fig. 11 according to one embodiment of the present invention, to make the next selection.

[00081] Returning to Fig. 8, control panel **630** provides functions to control imager **100** including recording video, capturing images, muting audio input, and confirming choices. Other functions as may be convenient and/or necessary may also be included.

[00082] To place device in recording mode to record a video file to a disk properly loaded in OMD **125**, user **10** touches the designated icon, here illustrated as icon **632**, in control panel icon **630**. In response, icon **632** may change design, such as becoming highlighted. Concurrently, in image panel **620**, image **25** is displayed in image window **624** and image status bar **622** displays confirmation of recording and elapsed recording as depicted in Fig. 12. Similarly if recording is initiated via CCU **30**, icon **632** becomes highlighted, image **25** is displayed in image window **624** and image status bar **622** displays confirmation of recording and elapsed recording, also as depicted in Fig. 12 according to one embodiment of the present invention. To cease recording, user **10** touches highlighted icon **632** or engages the appropriate control on CCU **30**.

- 29 -

[00083] To mute audio recording or conversely engage audio recording, user **10** touches the designated icon, here illustrated as icon **636**, in control panel **630**. In response, icon **636** may change design, such as becoming highlighted. To reverse the action, user **10** touches icon **636** which in response may change design, preferably returning to its previous design.

[00084] To capture an image that is being displayed in image window **624**, user **10** touches the designated icon, here illustrated as icon **634**, in control panel **630** and imager **100** is placed in image capture mode and the instruction is processed as described above. In response, icon **634** may change design, such as becoming highlighted, and a confirmation message that the desired action is being performed will be displayed. Similarly, image capture mode can be accessed if user **10** engages the appropriate control on CCU **30** to capture image **26** that is being displayed in image window **624**. Instruction is processed as described above and icon **634** may change design, such as becoming highlighted, and a confirmation message that the desired action is being performed will be displayed.

[00085] To allow user **10** to monitor available resources on a multimedia disc, multimedia status **610** includes fields identifying the remaining capacity of disc and the number of images captured and the length of time of image stream **25** recorded.

- 30 -

[00086] The archival mode is accessible from control panel **630** to review and/or manipulate saved documentary recording files and graphics file. User **10** touches the designated icon, here illustrated as icon **638**, and review page **440** is displayed as depicted in Fig. **13** according to one embodiment of the present invention. Page **440** preferably includes a control panel **630a**, note area **670**, file directory **660**, image panel **620** including image window **624**, image status bar **622**, and controls **626**. Controls **626** preferably include pause, playback, print and confirmation means as well as elapsed time and other controls as deemed useful and/or necessary.

[00087] Therein, a graphic file may be printed to printer **45** located in the surgical suite so that it is immediately available for review by user **10**. Software is provided to enlarge and view and manipulate the graphic file such as providing visual contrast, inserting a scaled file object corresponding to a physical prosthesis and thus determining whether such prosthesis fits patient **5**.

[00088] In accordance with one embodiment of the present invention, sensor **318** (see FIG. 4) is provided for detecting an infrared remote control signal. Sensor **318** enables user **10** to remotely operate imager **100**. Sensor **318** is in communication with the processor or Microprocessor main

- 31 -

board (MMB) **115**, the sensor receiving control signals to operate the medical instrument.

[00089] In accordance with one embodiment of the present invention, a system for speech recognition is provided for user **10** interaction with imager **100**. Microphone **40** receives user **10** voice commands, which are routed to speech recognition module **319**. Speech recognition module **319** is software that executes on Microprocessor main board (MMB) **115** to receive voice signals that control the medical instrument.

[00090] In accordance with one embodiment of the present invention, database module **321** provides a database server and/or database management application that is operatively provided to enable user **10** to access, manage and/or update data in imager **100**. Database module **321** is software that executes on Microprocessor main board (MMB) **115** to establish control signals to operate the hard drive and the optical media drive.

[00091] In accordance with one embodiment of the present invention, expert system **323** is provided wherein characteristics of video signal **300** meeting predetermined characteristics are automatically brought to the attention of user **10** and/or saved as graphic files **810**. Expert system **323**

- 32 -

is software that executes on Microprocessor main board (MMB) 115 to generate control signals to operate the medical instrument.

[00092] In accordance with one embodiment of the invention, a stereoscopic module 324 is provided for associating a plurality of video signals 300 with each other, as such providing stereoscopic images on a display unit. Stereoscopic module 324 is software that executes on Microprocessor main board (MMB) 115 to associate a plurality of files to provide stereoscopic images on a multimedia interface.

- 33 -

What is claimed is:

1. A device for medical video recording comprising:
an endoscope;
a digital media; and
an imager in communication with said endoscope, said imager converting energy received from said endoscope to signals that are contemporaneously stored onto said digital media.
2. The device of claim 1 further comprising an encoder in communication with said imager, said encoder compressing said signals.
3. The device of claim 1 wherein said media is an optical disc.
4. The device of claim 3 wherein said media is a digital versatile disk.
5. The device of claim 4 wherein said stored signals are stored as VOB files.
6. The device of claim 2 wherein said encoder is an MPEG encoder.
7. The device of claim 1 wherein said imager is a solid state device.
8. The device of claim 1 wherein said imager includes a still frame grabber.
9. The device of claim 8 wherein said imager stores still frames on said media.
10. The device of claim 1 further including a touch screen for entering control commands for said imager and said endoscope and said touchscreen is responsive to a touch by a user.

- 34 -

11. The device of claim 10 further including a housing, said housing enclosing said imager.

12. The device of claim 11 wherein said touch screen is at least partially retractable within a footprint of said housing.

13. The device of claim 11 wherein the touch screen is slidable at least partially out of a footprint of said housing.

14. The device of claim 11 wherein the touch screen is deflectable relative to said housing.

15. The device of claim 11 wherein the touch screen is pivotable relative to said housing.

16. The device of claim 10 wherein said touch screen displays said signal.

17. The device of claim 1 wherein said signal is electromagnetic energy.

18. The device of claim 1 wherein said signal is direct current energy.

19. A medical instrument having touch screen control comprising:

a touch screen for entering control commands;

a processor for receiving said control commands and for generating control signals to operate said medical instrument; and

a housing for enclosing said processor; said touch screen movable between a first position at least partially within a footprint of said housing and a second position extended from said footprint of said housing.

- 35 -

20. The medical instrument of claim 19 in which said touch screen is unpluggable from said housing.
21. The medical instrument of claim 19 in which said housing and said touch screen include stackable mating plug portions.
22. The medical instrument of claim 20 in which said touch screen can be used by a plurality of medical instruments.
23. The medical instrument of claim 19 in which said touch screen is deflectable about an axis of said housing.
24. The medical instrument of claim 23 in which said touch screen is easier to deflect in one direction than in the other direction.
25. The medical instrument of claim 23 in which said touch screen is more difficult to deflect in the opening direction than in the closing direction to permit said touch screen to be tapped without unintentionally deflecting said touch screen.
26. The medical instrument of claim 19 in which said touch screen presents a keyboard to a user.
27. The medical instrument of claim 19 further comprising a sensor in communication with said processor, said sensor receiving control signals to operate said medical instrument.

- 36 -

28. The medical instrument of claim 19 further comprising a speech recognition module executing on said processor, said speech recognition module receiving voice signals that control said medical instrument.

29. The medical instrument of claim 19 further comprising a expert system executing on said processor, said expert system generating control signals to operate said medical instrument.

30. The medical instrument of claim 19 in which said touch screen slides out of said housing.

31. The medical instrument of claim 19 in which said touch screen slides out of said housing and is deflectable.

32. A video recording and image capture device for recording data comprising:

a main board;

a first and second bus in communication with said main board;

an interface operable to receive a signal and forward the signal to said first bus;

an imager in communication with said main board, said imager recording said signal while contemporaneously writing said signal, said imager operably connected to said second bus; and

a touch screen connected to said second bus and responsive to a touch by a user, said touch screen for entering control commands for said interface.

- 37 -

33. The device of claim 32 wherein said interface is operable to receive and process said signal into an MPEG stream, said interface connected on said first bus to the main board.

34. The device of claim 32 and 33 wherein said imager records and writes said files as an MPEG stream.

35. The device of claim 32 further comprising a database module executing on said main board, said database module structuring storage of said files.

36. The device of claim 32 further comprising a sensor in communication with said main board, said sensor generating control signals to operate said device.

37. The device of claim 32 further comprising a speech recognition module executing on said main board, said speech recognition module generating control signals to operate the device.

38. The device of claim 32 further comprising an expert system executing on said main board, said expert system generating control signals to operate said device.

39. The device of claim 32 further comprising a stereoscopic module executing on said main board, said stereoscopic module associating a plurality of files to provide stereoscopic images on said interface.

40. The device of claim 32 wherein said interface comprises at least one relay to route an input signal to a corresponding output connector for providing an output signal regardless of the operation status of said device.

- 38 -

41. An interface for processing a signal for recording video into a multiple frame layer comprising:

a controller for an inter-ic bus for providing a multiple master digital connection;

an analog to digital converter for converting a video signal to a first digital stream, said converter operably connected to said inter-ic bus;

a video compression and decompression integrated circuit for encoding said first digital stream into a second digital stream having frames, and decoding said second digital stream, said video compression and decompression integrated circuit operably connected to said inter-ic bus; and

a programmable buffer for selectively saving frames handled by said controller, said buffer operably connected to said controller and said video compression and decompression integrated circuit, and said buffer inserting said frames into said second digital stream for decoding.

42. A method for recording an MPEG file for documenting surgical procedures while displaying an MPEG stream and a plurality of selected still image files corresponding to the MPEG stream, comprising the steps of:

providing a first digital data stream comprising a video signal,

providing a second digital data stream comprising an audio signal,

multiplexing an MPEG data stream from said first and second digital data stream,

- 39 -

streaming said MPEG data stream to an imager operably connected on a bus;

writing said MPEG stream to said imager;

displaying said MPEG stream on a display unit;

selecting a number of frames from said MPEG stream;

converting the frames to still image files; and

multiplexing a signal to said display unit by adding the still image files.

43. The method of claim 42 in which said still image files are in JPEG format.
44. The method of claim 42 in which said still image files are in BMP format.
45. The method of claim 4 in which the still image files are in TIFF format.

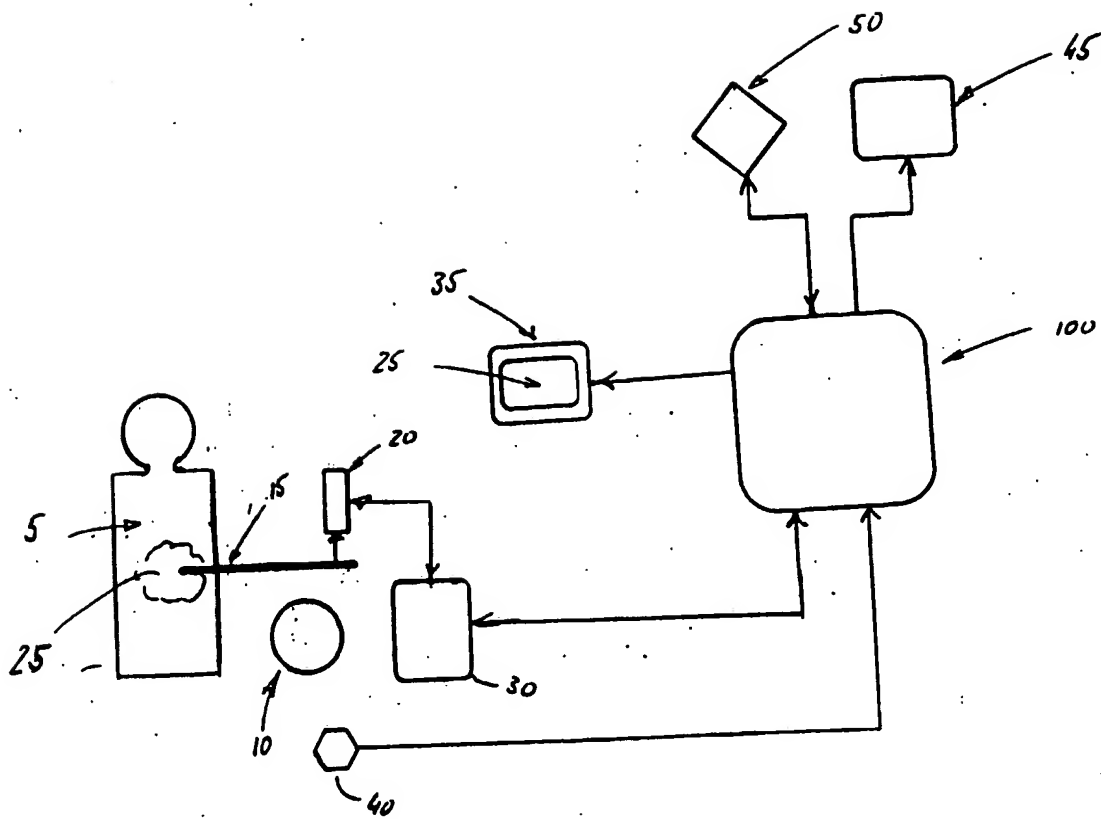
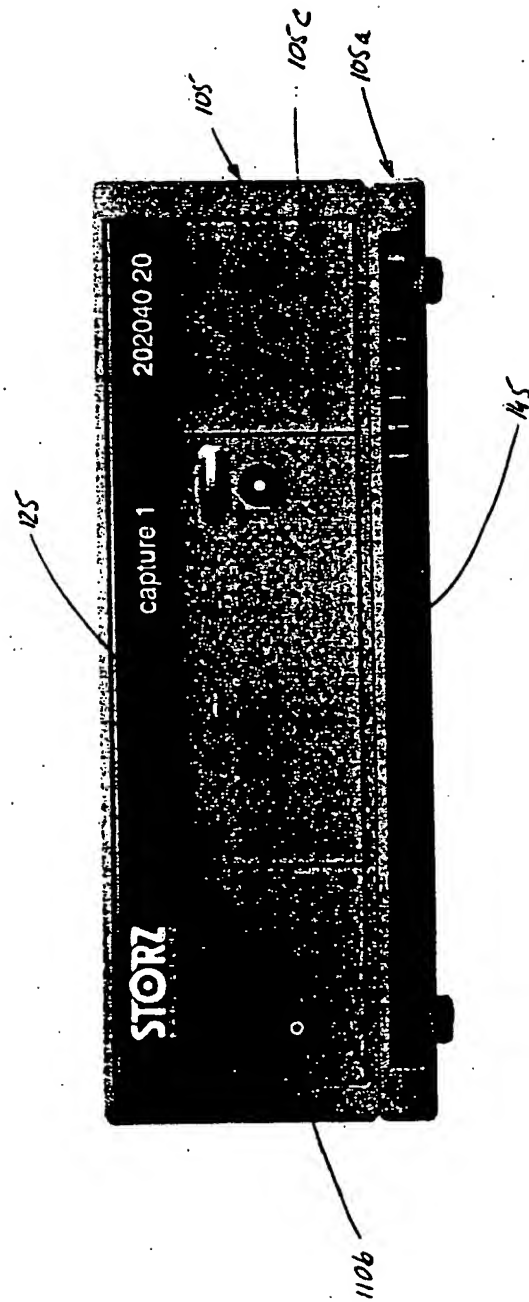


Fig. 1



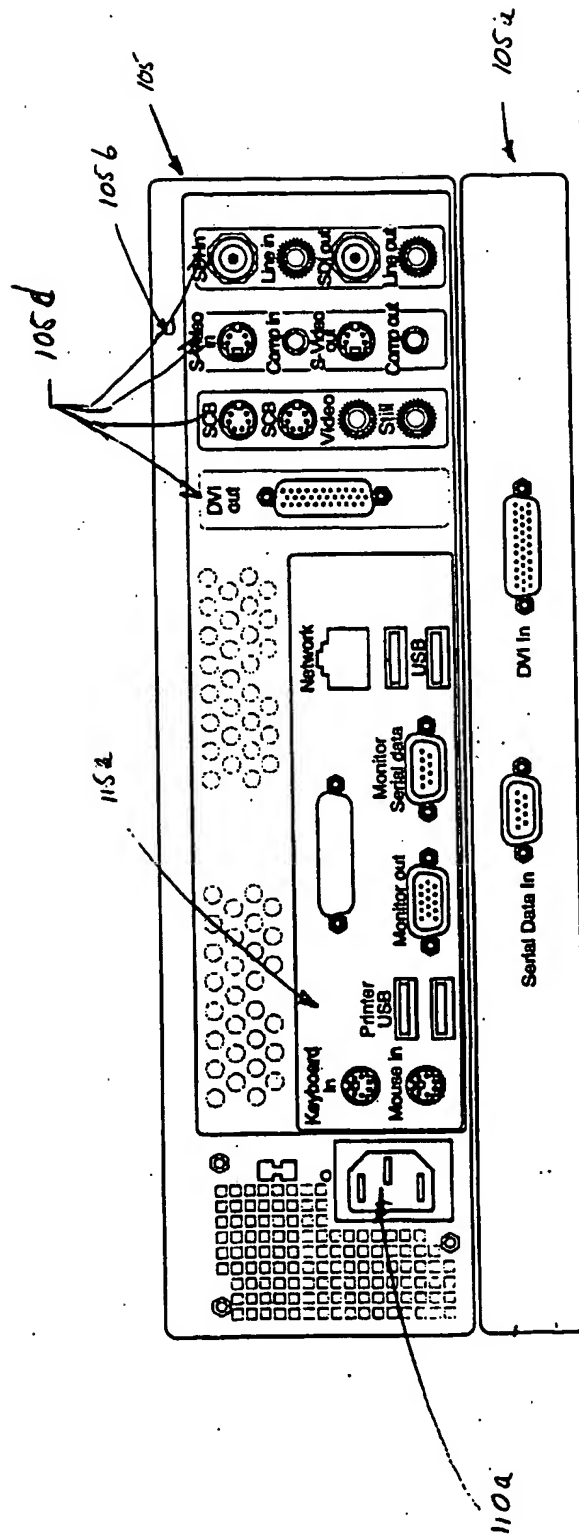


Fig. 3.

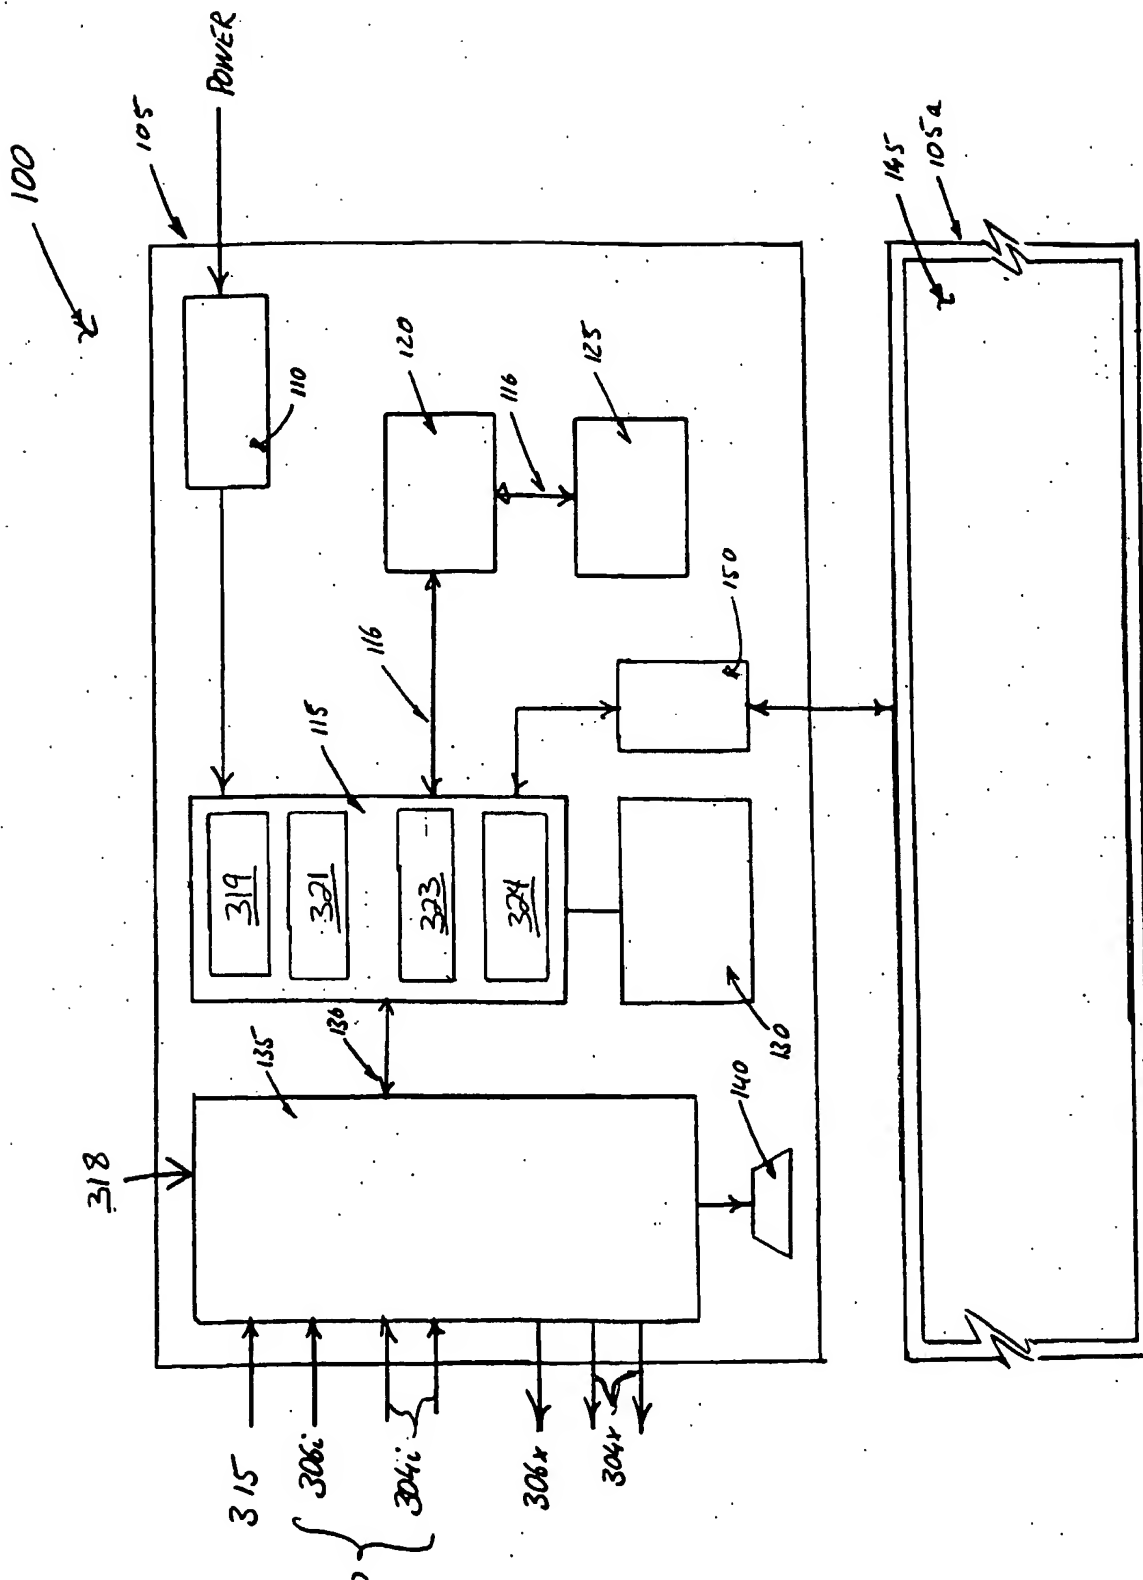


FIG. 4

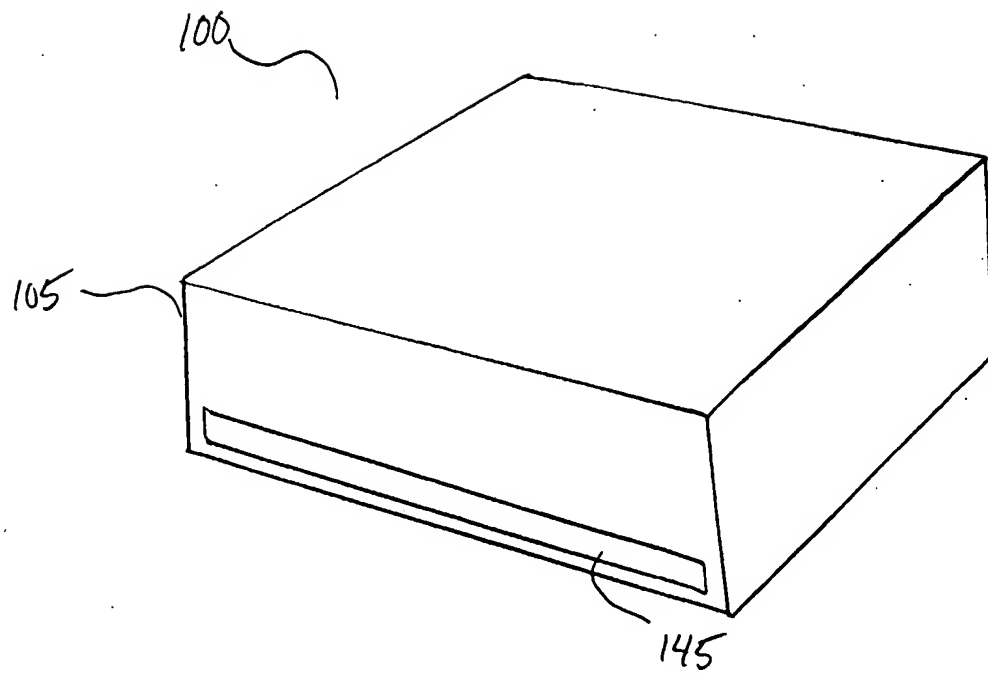


Fig. 5a

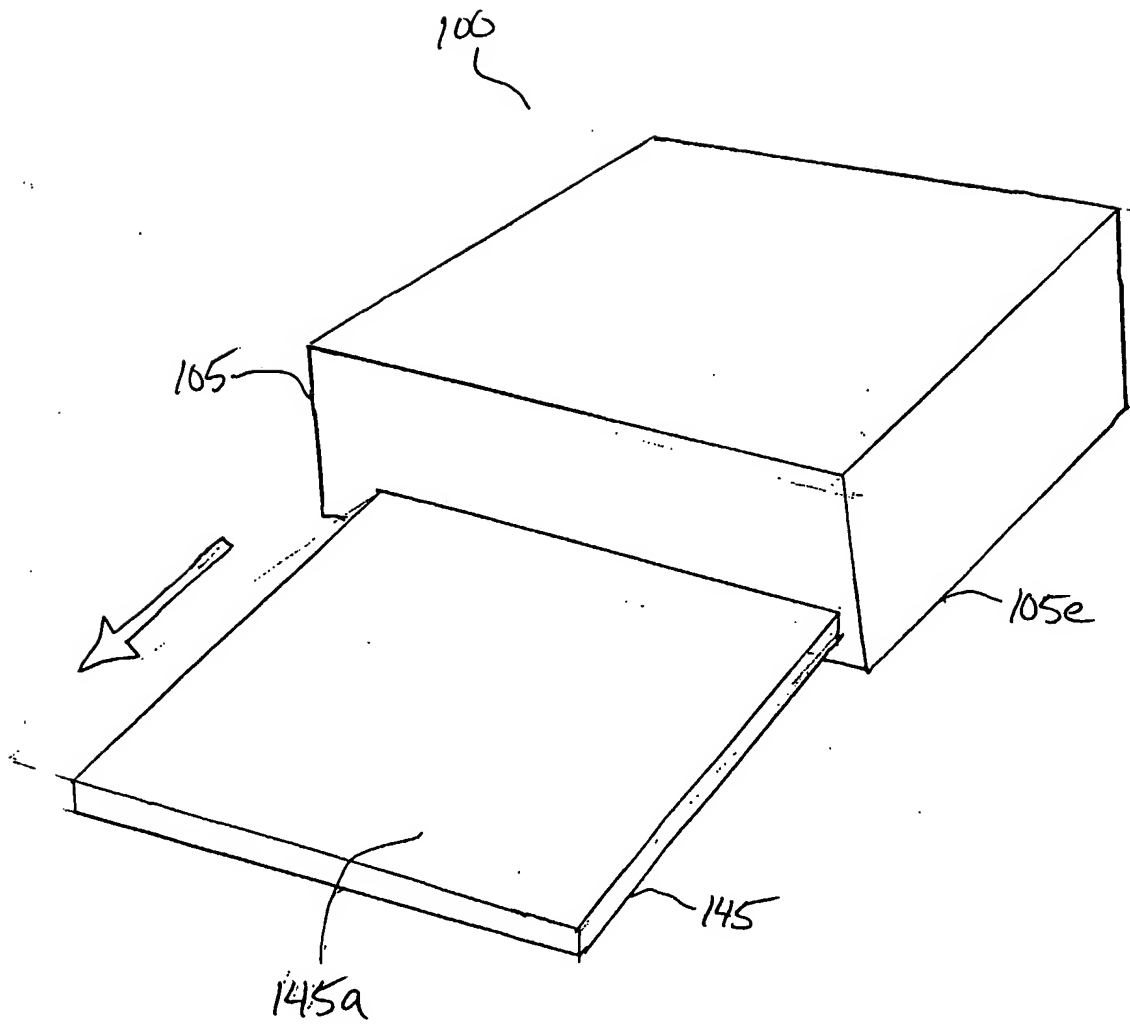


Fig 5b

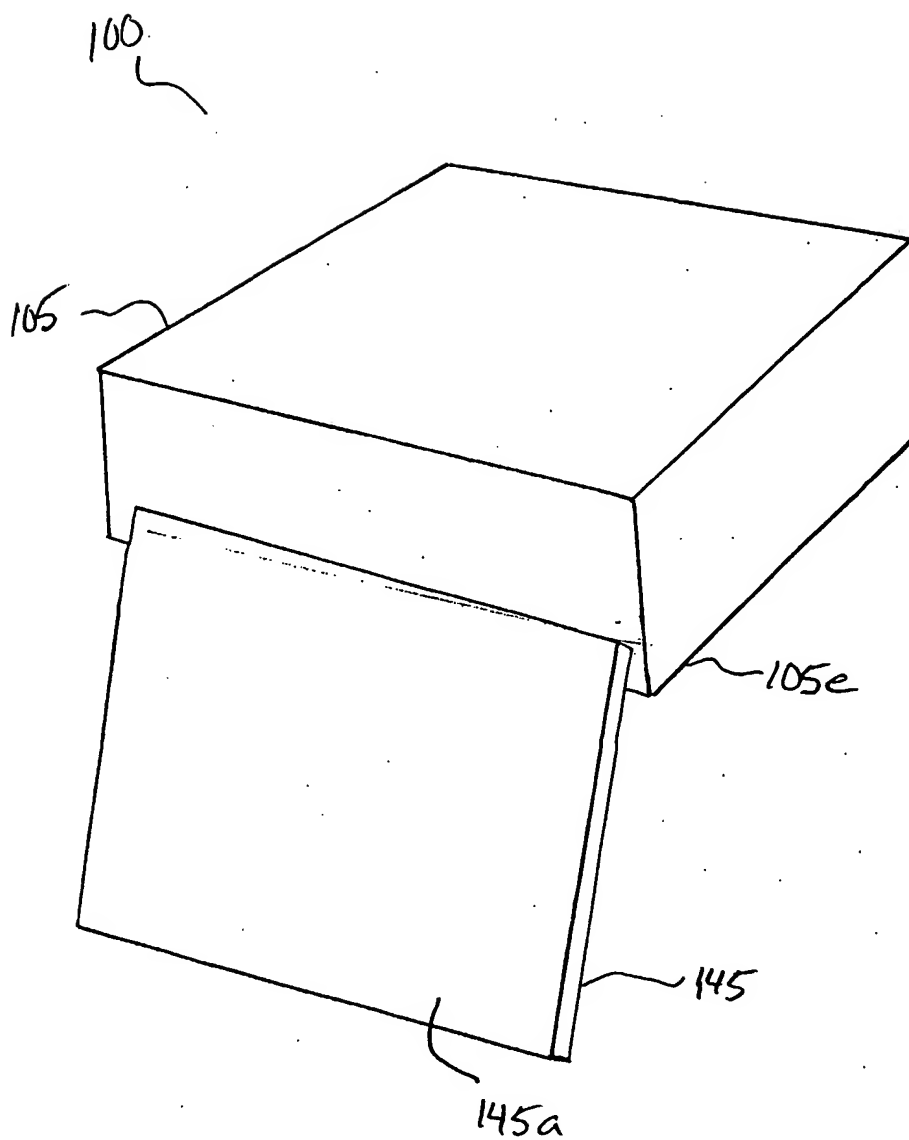


Fig. 5c

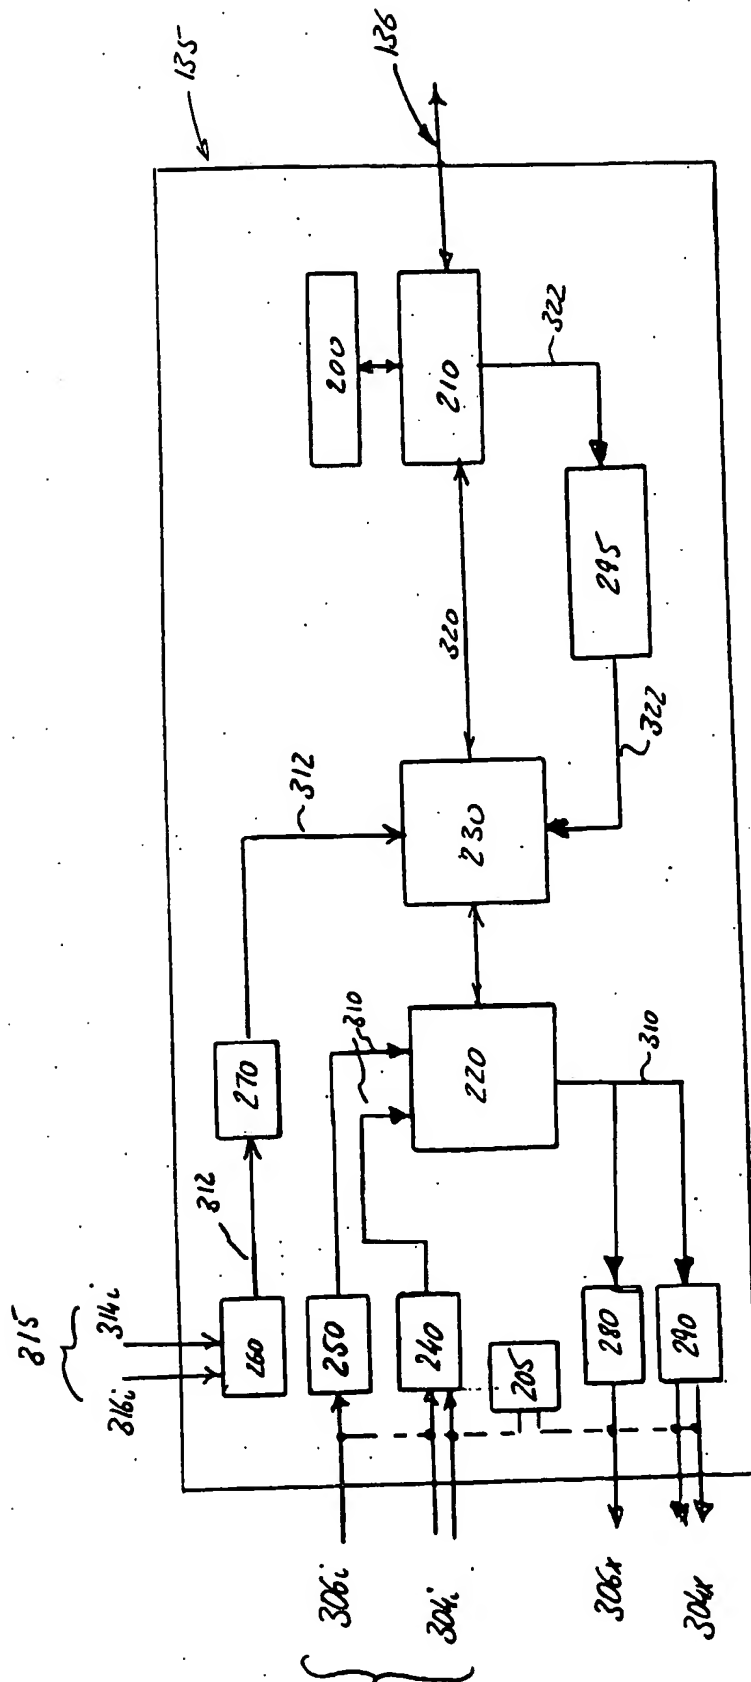


Fig. 6

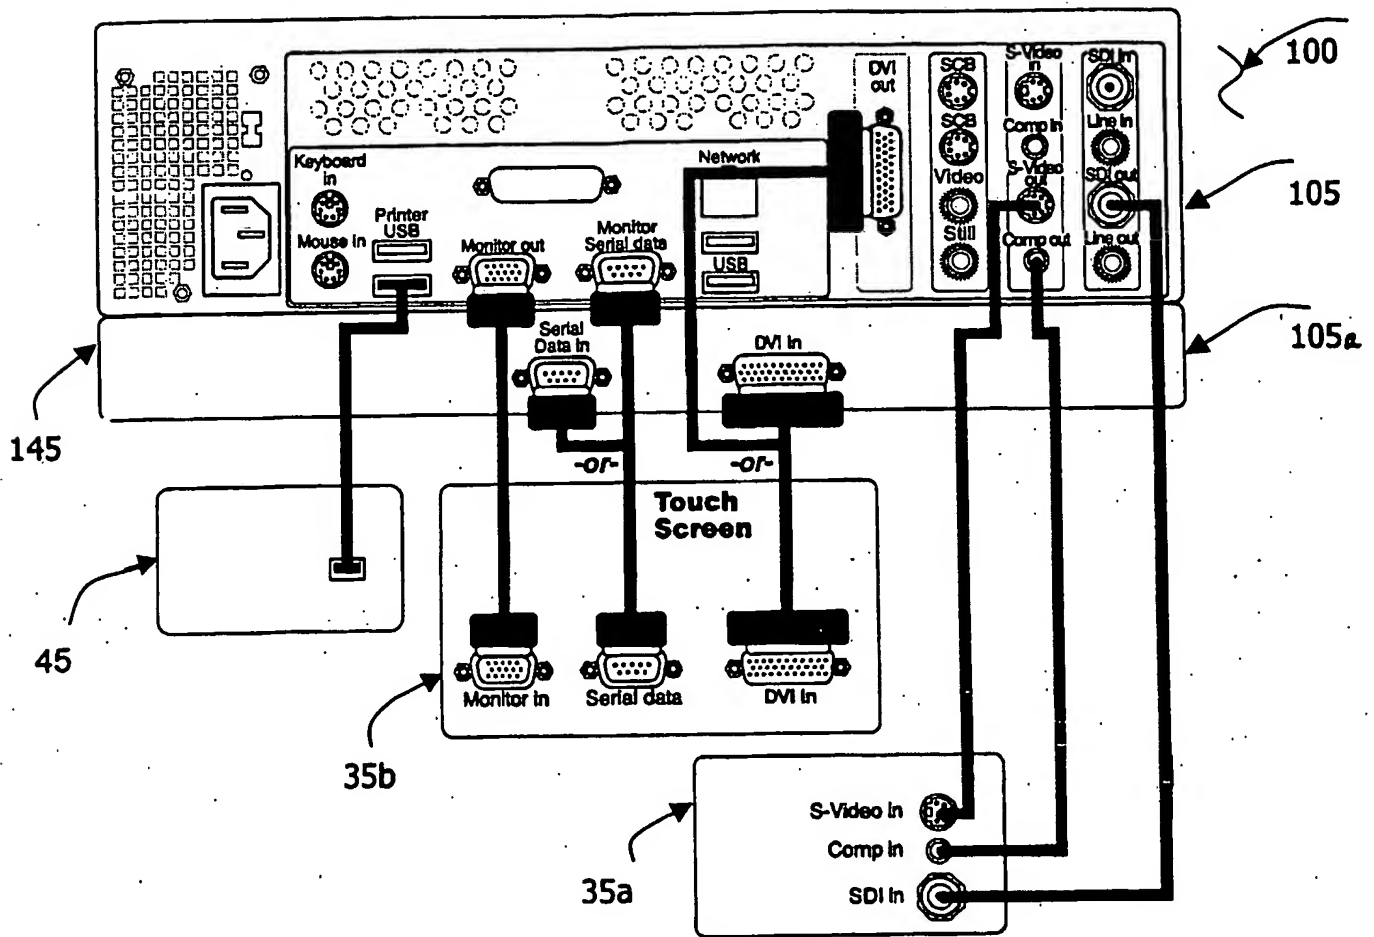


Fig. 7

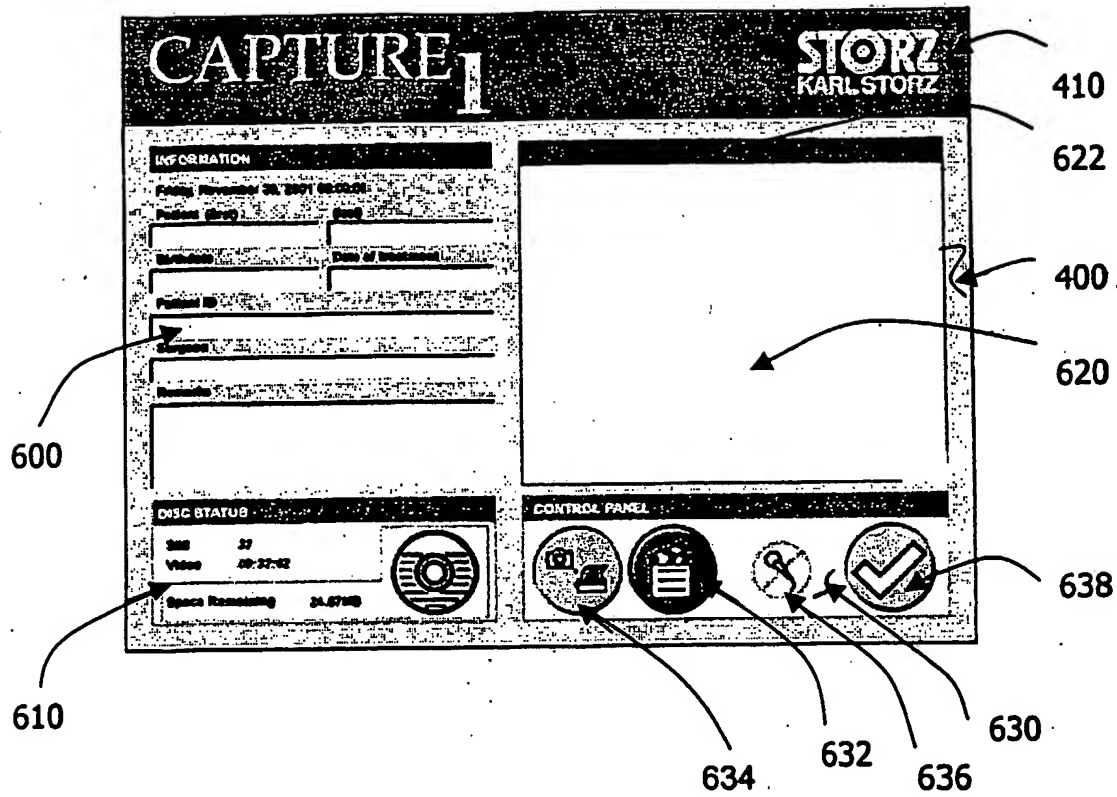


Fig. 8

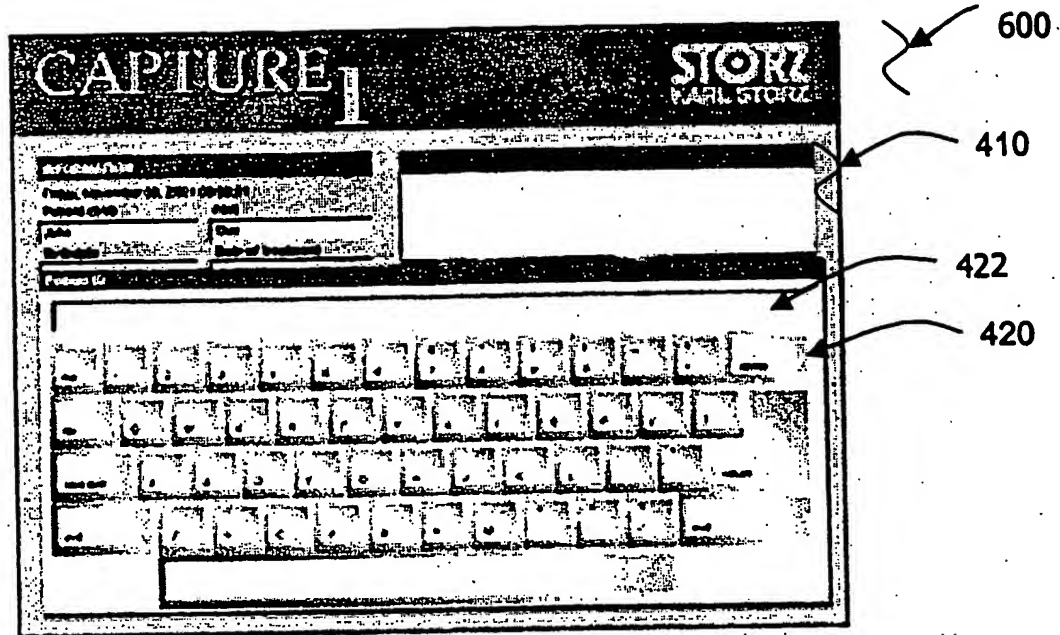


Fig. 9

CAPTURE I

STORZ
KARL STORZ

INFORMATION

Patient name: [Field]
 Date: [Field]
 Date of capture: [Field]

NOTES

[Text Area]
 PRINT

CAPTURE

Grid of buttons: 1, 2, 3, 4, 5, 6, 7, 8, 9, 0, CHECK

400

432

430

410

Fig. 10

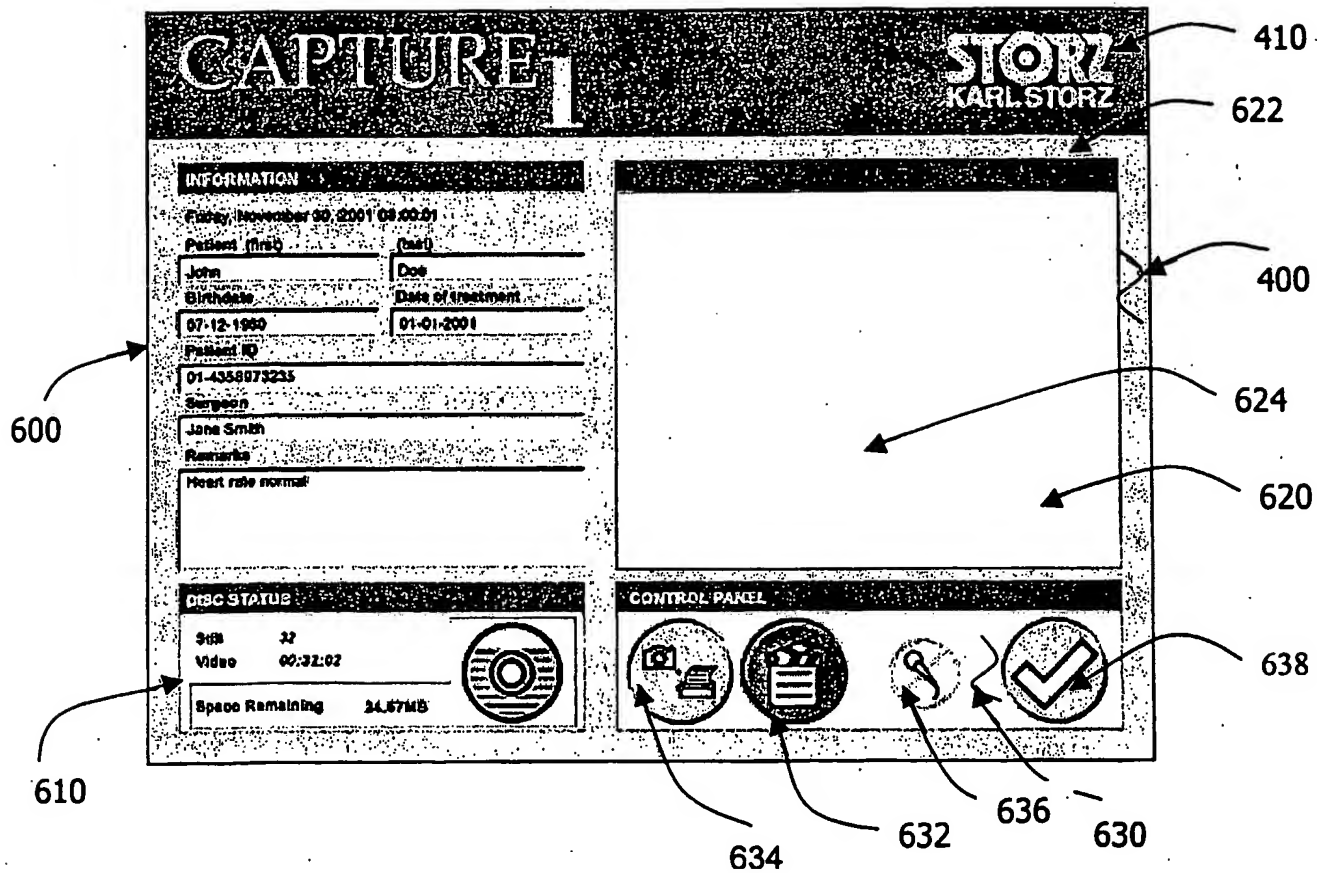


Fig. 11

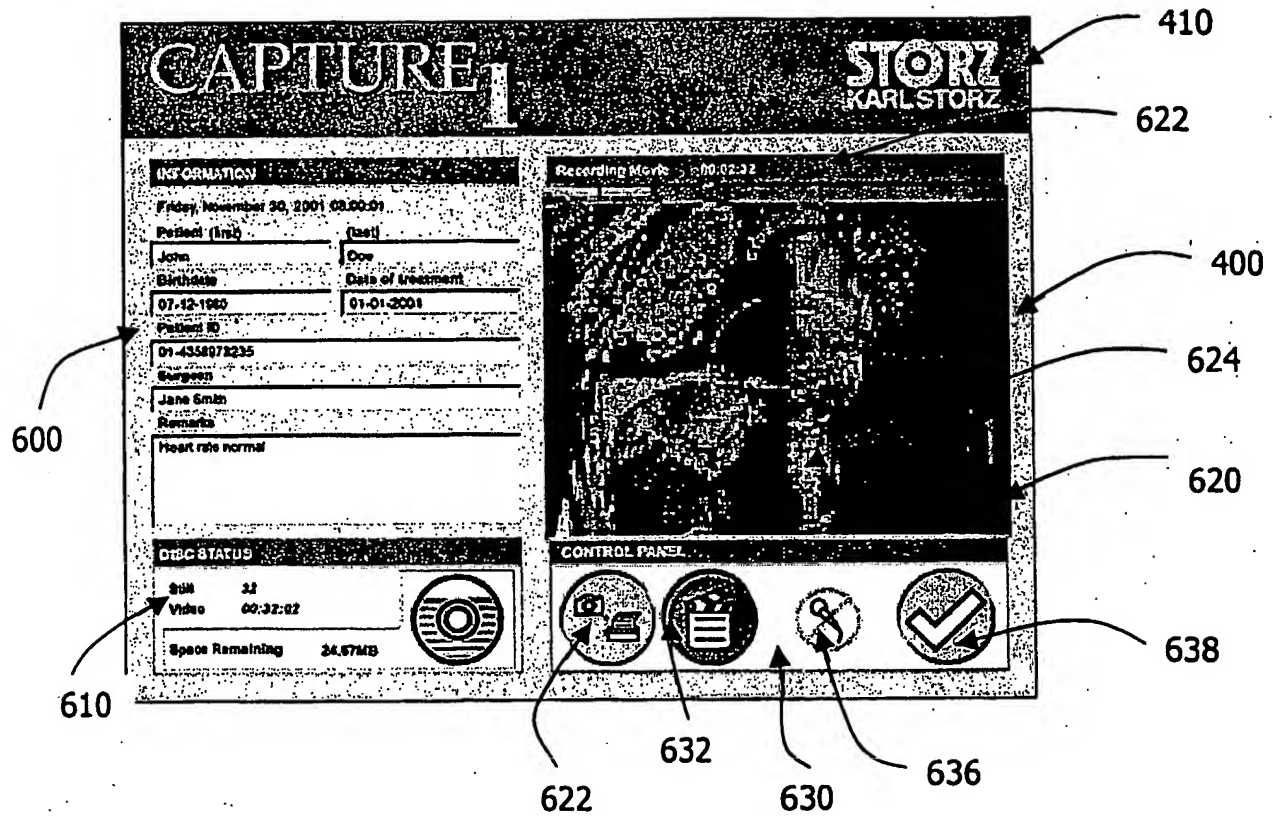


Fig. 12

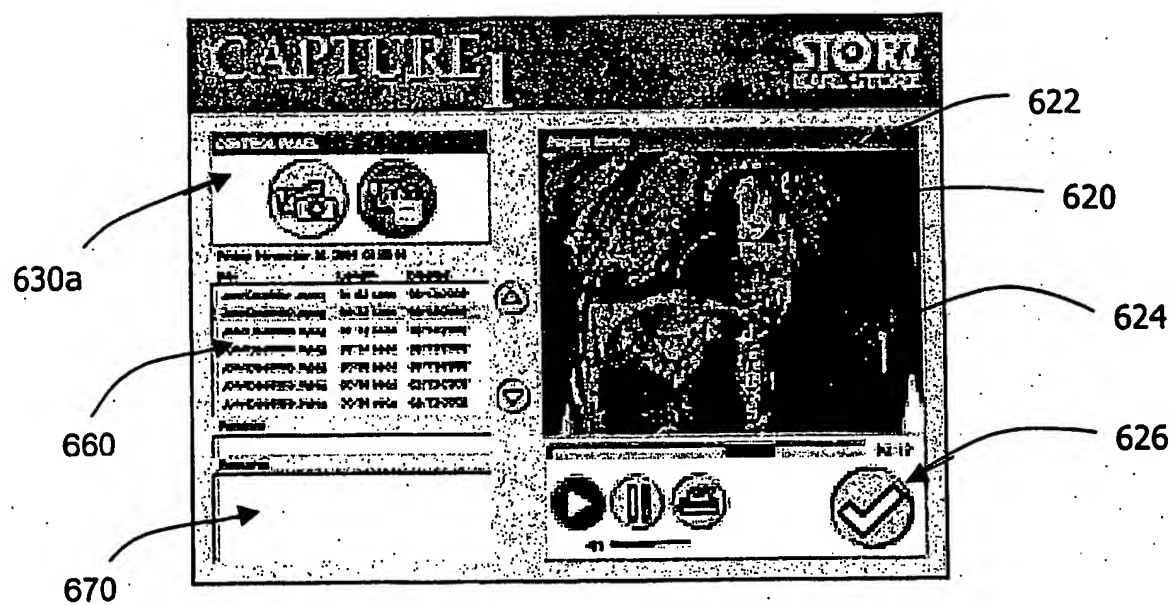


Fig. 13

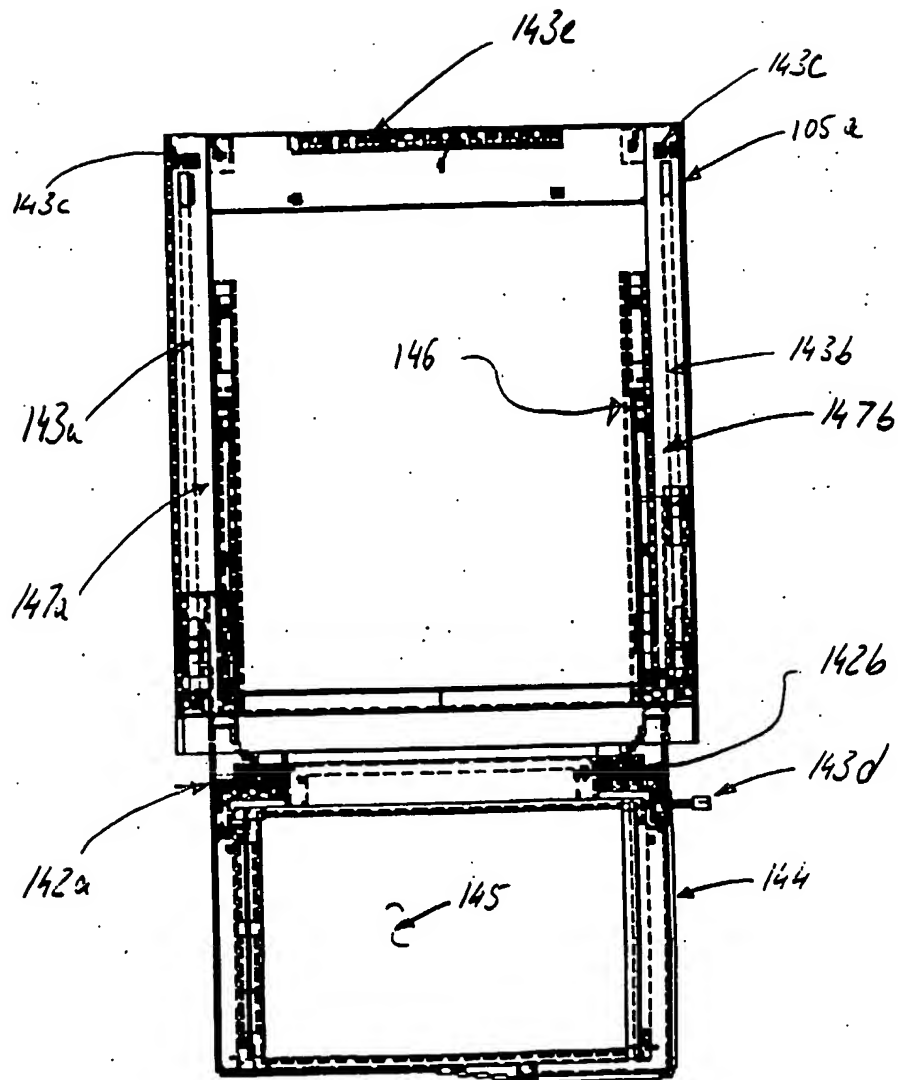


Fig. 14a

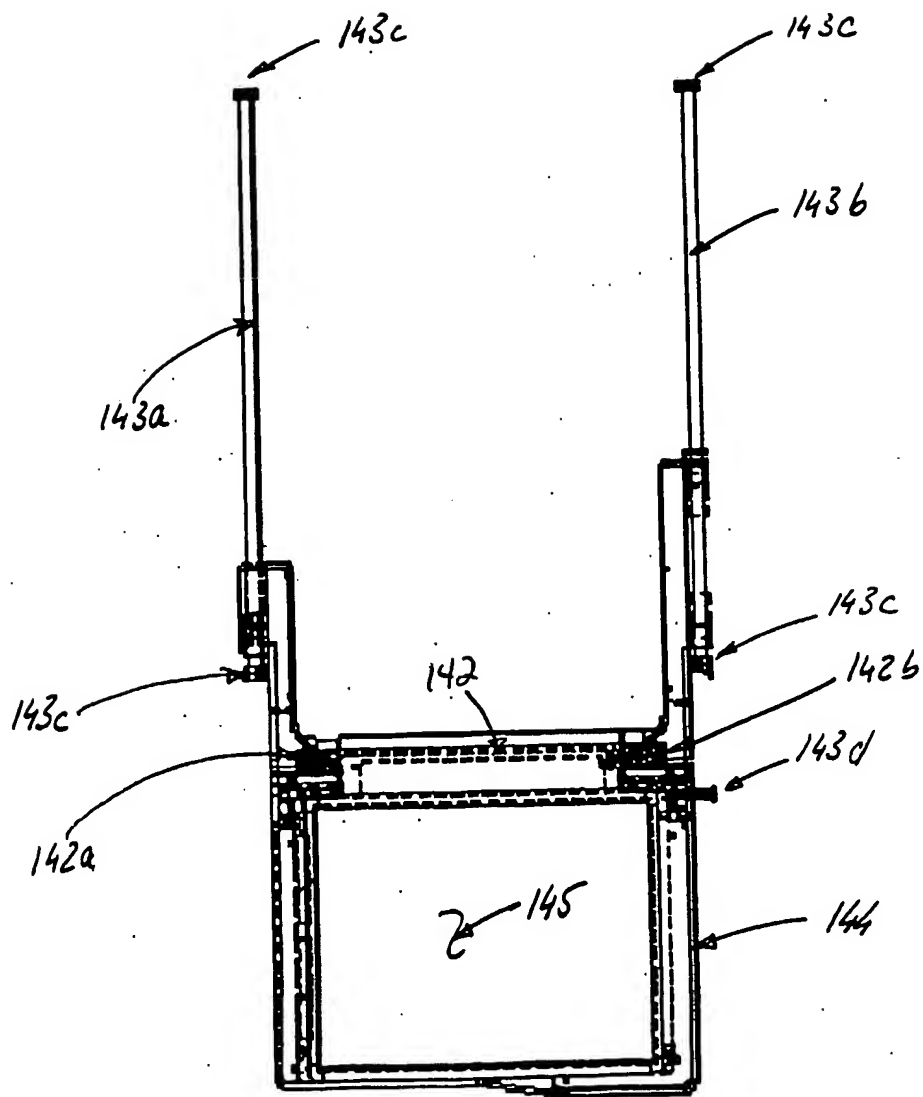


Fig. 146

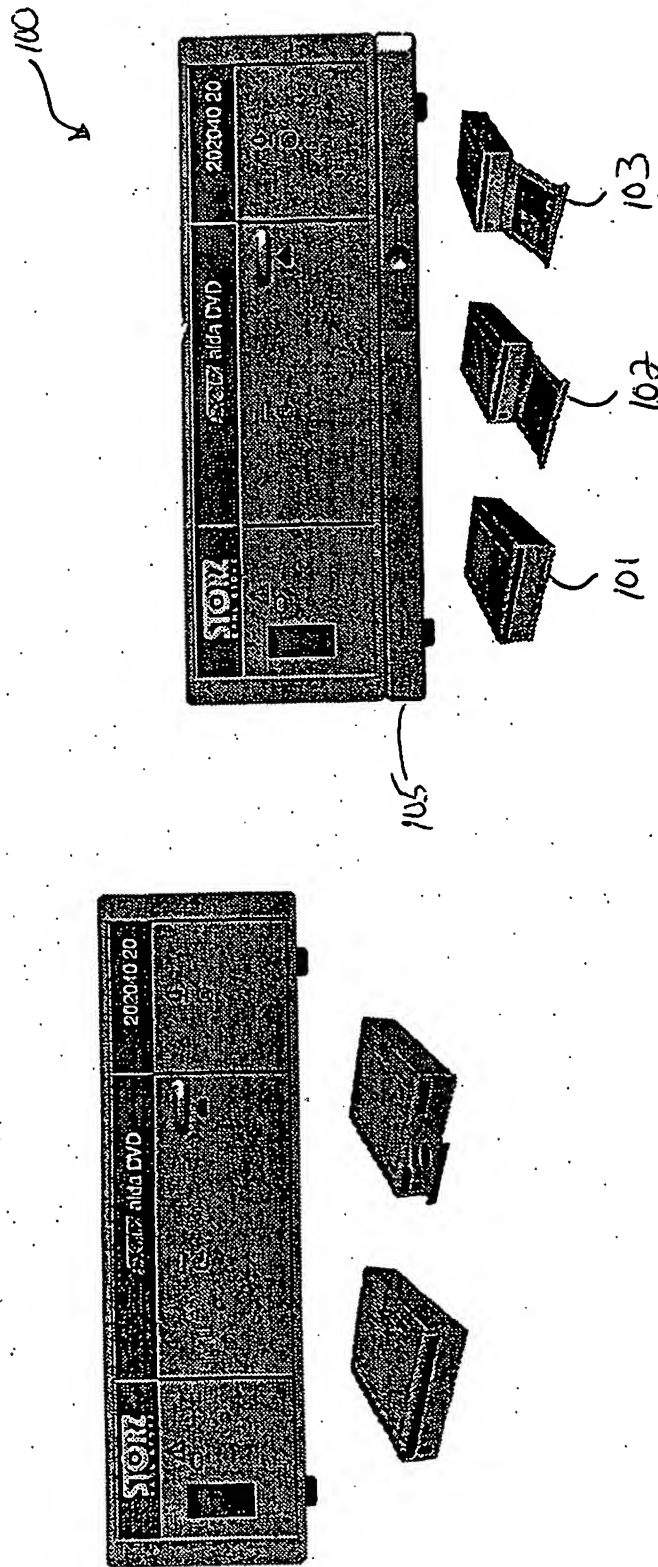


Fig. 15

INTERNATIONAL SEARCH REPORT

International application No.

PCT/US03/29012

A. CLASSIFICATION OF SUBJECT MATTER

IPC(7) : H04N 7/18, 9/47; A62B 01/04

US CL : 348/65

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

U.S. : 348/65

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)
East

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X,P	US 6,471,649 B1 (SACCARDO et al) 29 October 2002 (29.10.2002) figure 5 and figure 3	1-45
X	US 6,184,922 B1 (SAITO et al) 06 February 2001 (06.02.2001) Figures 2-5 and columns 3-28	1-45

☐

Further documents are listed in the continuation of Box C.

☐

See patent family annex.

* Special categories of cited documents:	*T* later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
A document defining the general state of the art which is not considered to be of particular relevance	*X* document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
E earlier application or patent published on or after the international filing date	*Y* document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art
L document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)	*Z* document member of the same patent family
O document referring to an oral disclosure, use, exhibition or other means	
P document published prior to the international filing date but later than the priority date claimed	

Date of the actual completion of the international search

20 January 2004 (20.01.2004)

Date of mailing of the international search report

28 JAN 2004

Name and mailing address of the ISA/US

Mail Stop PCT, Attn: ISA/US
Commissioner for Patents
P.O. Box 1450
Alexandria, Virginia 22313-1450

Facsimile No. (703)305-3230

Authorized officer

Chris Kelley

Telephone No. 703-305-4750